

[illegible]

FIG. 2


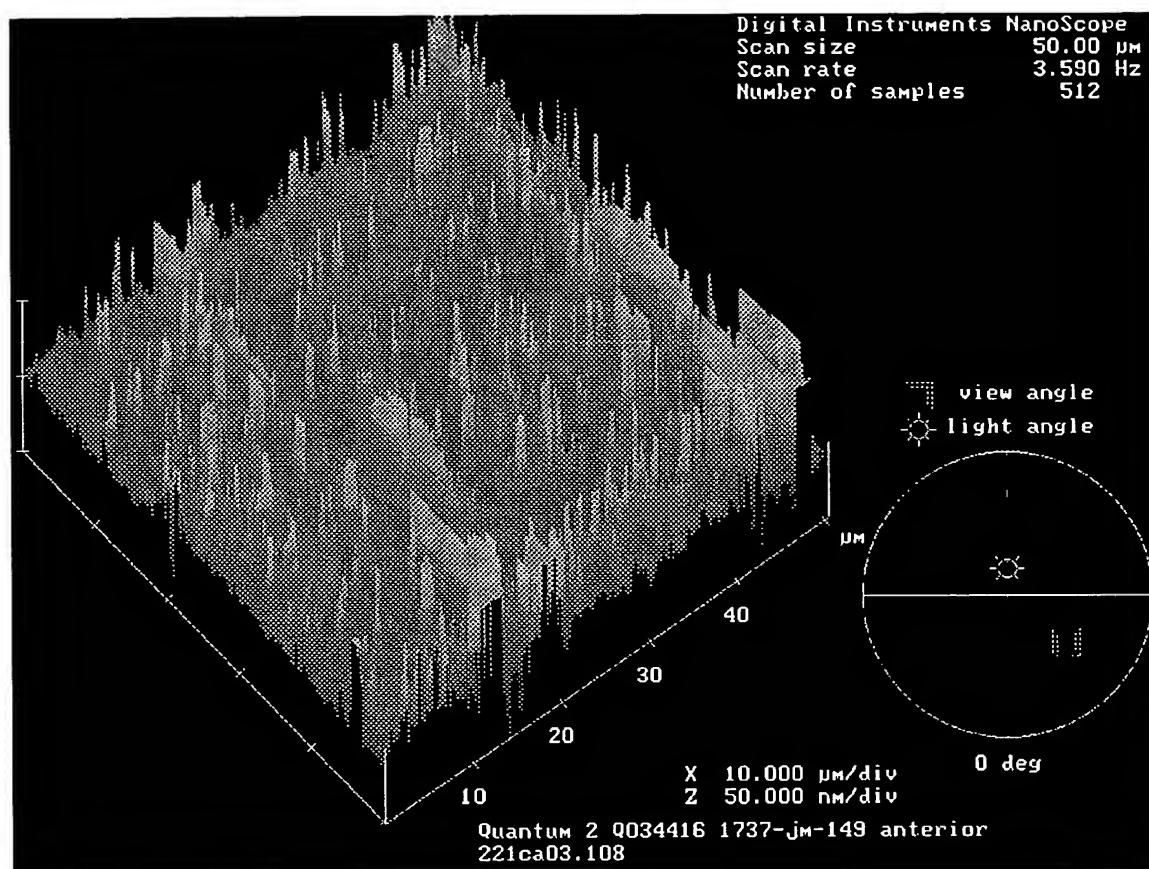


FIG. 3

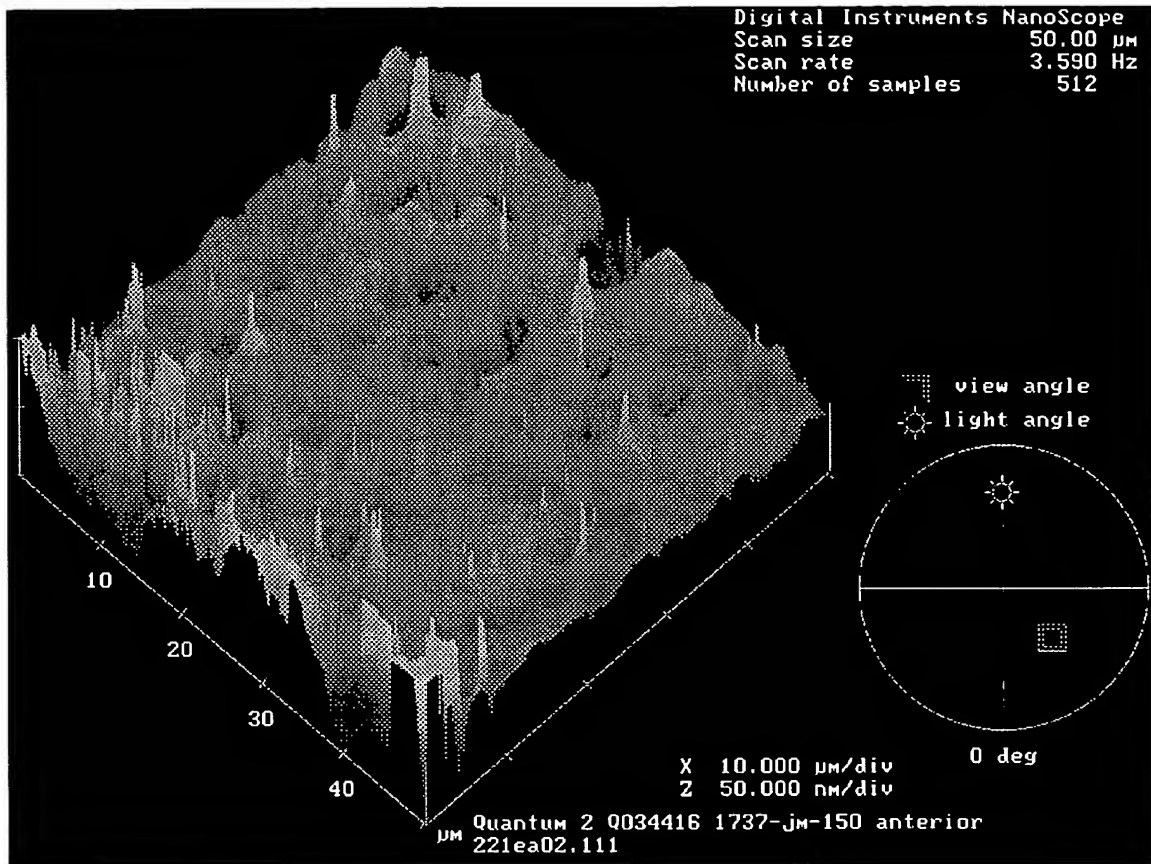

1000550-10804

FIG. 4 (Control)

Digital Instruments NanoScope
Scan size 50.00 μm
Scan rate 3.052 Hz
Number of samples 512

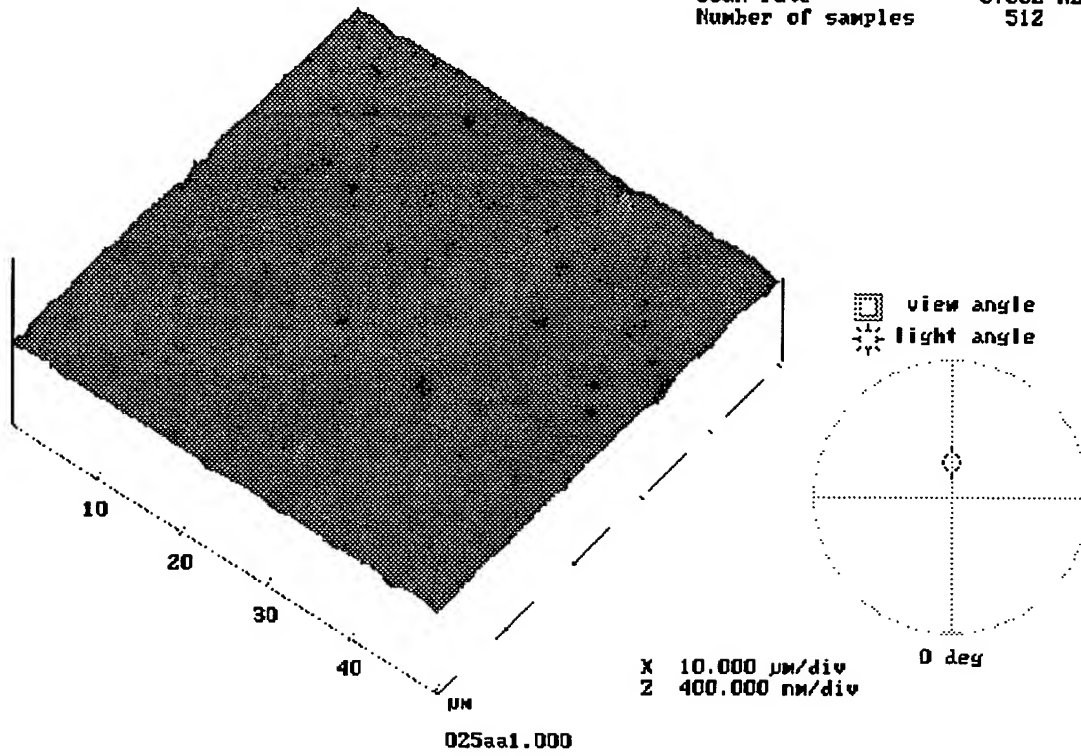


FIG. 5

Digital Instruments NanoScope
 Scan size 50.00 μm
 Scan rate 3.391 Hz
 Number of samples 256
 Image Data Height
 Data scale 400.0 nm

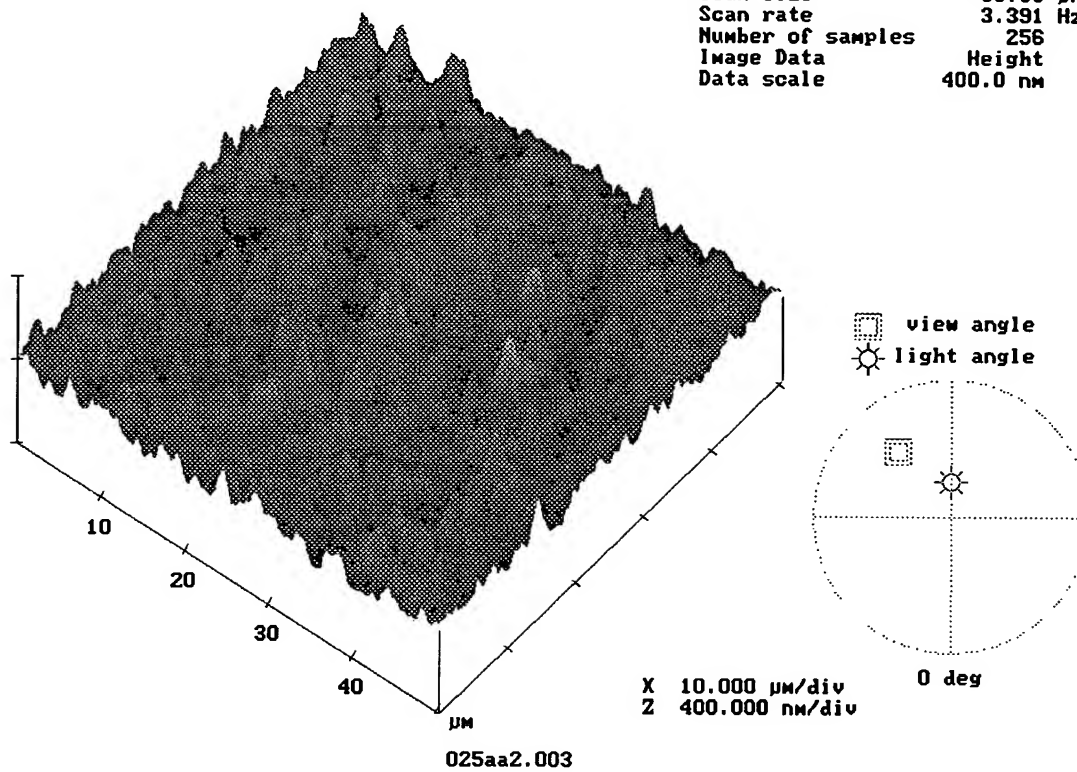


FIG. 6

10005560-1100004

